

CS505 FUEL MOISTURE SENSOR INSTRUCTION MANUAL

6/98

COPYRIGHT (c) 1998 CAMPBELL SCIENTIFIC, INC.

WARRANTY AND ASSISTANCE

The **CS505 FUEL MOISTURE SENSOR** is warranted by CAMPBELL SCIENTIFIC, INC. to be free from defects in materials and workmanship under normal use and service for twelve (12) months from date of shipment unless specified otherwise. Batteries have no warranty. CAMPBELL SCIENTIFIC, INC.'s obligation under this warranty is limited to repairing or replacing (at CAMPBELL SCIENTIFIC, INC.'s option) defective products. The customer shall assume all costs of removing, reinstalling, and shipping defective products to CAMPBELL SCIENTIFIC, INC. CAMPBELL SCIENTIFIC, INC. will return such products by surface carrier prepaid. This warranty shall not apply to any CAMPBELL SCIENTIFIC, INC. products which have been subjected to modification, misuse, neglect, accidents of nature, or shipping damage. This warranty is in lieu of all other warranties, expressed or implied, including warranties of merchantability or fitness for a particular purpose. CAMPBELL SCIENTIFIC, INC. is not liable for special, indirect, incidental, or consequential damages.

Products may not be returned without prior authorization. To obtain a Returned Materials Authorization (RMA), contact CAMPBELL SCIENTIFIC, INC., phone (435) 753-2342. After an applications engineer determines the nature of the problem, an RMA number will be issued. Please write this number clearly on the outside of the shipping container. CAMPBELL SCIENTIFIC's shipping address is:

CAMPBELL SCIENTIFIC, INC.

RMA# _____

815 West 1800 North
Logan, Utah 84321-1784

CAMPBELL SCIENTIFIC, INC. does not accept collect calls.

Non-warranty products returned for repair should be accompanied by a purchase order to cover the repair.



CAMPBELL SCIENTIFIC, INC.

815 W. 1800 N.
Logan, UT 84321-1784
USA
Phone (435) 753-2342
FAX (435) 750-9540
www.campbellsci.com

Campbell Scientific Canada Corp.
11564 -149th Street
Edmonton, Alberta T5M 1W7
CANADA
Phone (403) 454-2505
FAX (403) 454-2655

Campbell Scientific Ltd.
Campbell Park
80 Hathern Road
Shepshed, Leics. LE12 9RP
ENGLAND
Phone (44)-50960-1141
FAX (44)-50960-1091

CS505 FUEL MOISTURE SENSOR

1. GENERAL DESCRIPTION

The CS505 Fuel Moisture Sensor provides an automated measurement of the moisture content of a standard 10-hour fuel moisture dowel. The moisture content of the 10-hour fuel sensor represents the moisture content of small-diameter (10-hour time lag) forest fuels.

Traditionally, the standard fuel moisture stick consists of a rack of four 1/2 inch diameter ponderosa pine dowels. The resulting rack is about 20 inches long with an oven-dry weight of 100 grams. The characteristic time constant of the rack is 10 hours. The rack is mounted 12 inches or about 30 centimeters above the forest floor. The rack is left outside continually exposed to the same conditions as forest fuels. The rack absorbs and desorbs moisture from its surroundings. As the rack transfers moisture, its weight changes. Periodic weighing of the rack determines changes in moisture content provides an indication of moisture changes in forest fuels.

The CS505 sensor incorporates the same carefully selected USFS standard ponderosa dowels as the traditional weighing fuel moisture racks. No artificial materials (e.g., epoxy sealant) are added to the dowel that would adversely influence the natural behavior characteristics of the dowel. Because the complete dowel surface is accessible for moisture exchange, the response of the CS505 is similar to that of the traditional weighing racks. To optimize probe-to-probe repeatability and to allow probe interchangeability without individual calibration, two additional sorts are performed on the dowels before they are selected to be used as a sensor. First, the dowels are sorted dry by density to improve accuracy in the dry range of 0 to 15%. Second, the dowels are sorted after a 50-minute soak by weight to reduce probe-to-probe time response variation and minimize variability in the wet range of 20 to 50%.

Even after careful selection and sorting is performed to choose the most representative dowels, the majority of measurement error is due to the variability of wood. Wood's ability to transfer moisture is dependent on many variables, primarily cell structure and wood

resin content. These variables change over time and after repeated wetting and drying cycles. Only a small amount of overall measurement error is due to the electronic circuitry.

2. SPECIFICATIONS

The fuel moisture sensor consists of two stainless steel strips pressed into groves in a standard 1/2 inch ponderosa pine dowel and secured with nylon tie wraps. The probe connects to the electronics with two Phillips head screws. A shielded four-conductor cable is connected to the circuit board to supply power, enable the electronics, and monitor the signal output. The printed circuit board is encapsulated in a water proof epoxy housing.

High speed electronic components on the circuit board are configured to oscillate when power is applied. The output of the circuit is connected to the fuel moisture probe which acts as a wave guide. The oscillation frequency and therefore output signal of the circuit is dependent on the dielectric constant of the media surrounding the stainless steel strips. The dielectric constant is predominantly dependent on the water content of the wood. Digital circuitry scales the oscillation frequency to an appropriate range for measurement with a datalogger. The CS505 output is essentially a square wave with an amplitude of ± 2.5 VDC. The frequency of the square wave output ranges from approximately 600 to 1500 Hz.

***Fuel moisture accuracy:**
(with a new stick)

<u>range</u>	<u>90% of all measurements</u>	<u>rms error</u>
0 to 10%	$\pm 2\%$	$\pm 1.0\%$
10 to 20%	$\pm 3\%$	$\pm 1.5\%$
20 to 30%	$\pm 5\%$	$\pm 2.2\%$
30 to 50%	$\pm 6\%$	$\pm 2.4\%$

Range: 0-50%

Power Supply: 9 VDC minimum to 18 VDC maximum

Enable voltage: off at 0 V (<1 VDC)
on at 5 V (>1.5 VDC maximum 12 VDC)

CS505 FUEL MOISTURE SENSOR

Current usage: 70 mA active/ 10 uA quiescent

Output signal: ± 2.5 V square wave with an output frequency of approximately 600 to 1500 Hz.

Dimensions:

sensor: 1/2 inch dowel, 20 inch long
electronics: 4 x 2.5 x 0.75 inches

*The above accuracy is a static accuracy derived at slow changing conditions with experimental data.

3. INSTALLATION

As shown in Figure 1 and Figure 2, both the CS505 and CS205 install on the 10974 mounting stake. The probes install horizontally and should point south in the northern hemisphere and north in the southern. The rack is mounted above a representative forest-floor duff layer. The stake is carefully

hammered into the ground so that it is vertical. Don't hammer on the spot-welded clips that hold the CS505 electronics. Once the stake is installed, insert the CS505 electronics into the two spring clips. The fuel moisture sensor (part number 10824) installs on the CS505 electronics with the supplied Phillips-head screws. The CS205 fuel temperature stick is inserted into the mounting stake's compression fitting. The 107 temperature probe is then inserted into the CS205 stick. Tighten the compression fitting so that it compresses the split wood and snugly holds the 107 probe.

The mounting stake ships with a package of 12 ultraviolet light resistant cable ties. The mounting stake has five holes punched along the edge of the shaft. There are two pairs of holes higher and one single hole lower on the shaft. When the stake is inserted into the ground to a depth level with the lower hole, the probes are at 12 inches or about 30 centimeters above the ground surface. The two upper pairs of holes are used to attach two tie wraps per cable—one pair for both the CS505 and CS205/107.

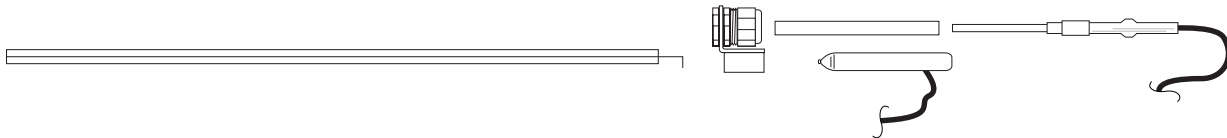


FIGURE 1. Exploded View of CS505 and CS205 Mounting

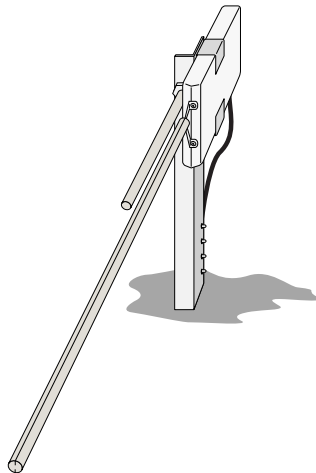


FIGURE 2. CS505 Installation Options Over Forest Floor, 30cm Over Duff Layer

4. WIRING

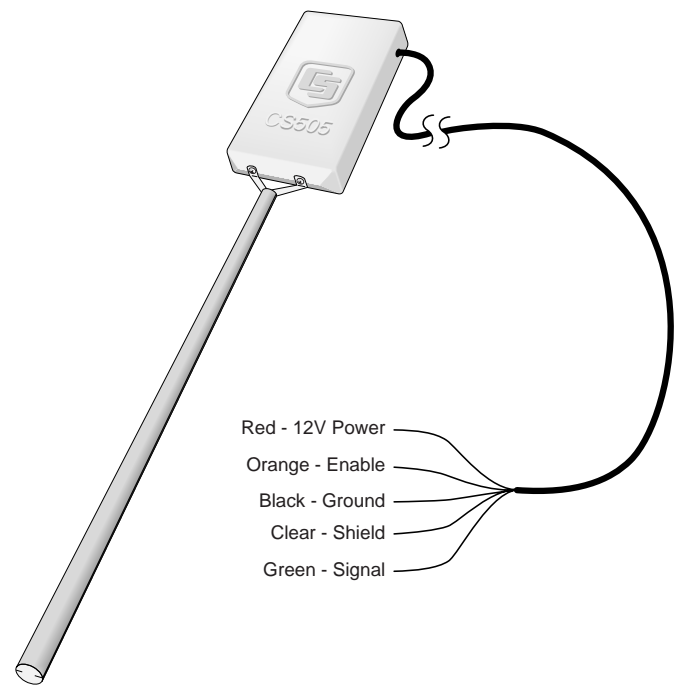


FIGURE 3. CS505 Wire Color and Function

color	function	CR10(X),CR500	21X/CR7	CR23X
red	power	12 V	12 V	12 V
black	ground	G	≠	G
green	signal	Analog Channel	Pulse Channel	Analog Channel
orange	enable	Control Port or Switched Excitation	Switched Excitation	Control Port or Switched Excitation
clear	ground	G	≠	≠

5. PROGRAMMING

The CS505 has a built in enable circuit. When voltage on the enable lead is less than 1.3 VDC, the sensor is off. When a voltage greater than 1.3 VDC, commonly 5 VDC, is applied to the enable lead, the sensor is on. The output signal is a ± 2.5 volt square wave. Instruction P27 Period Average in the CR500, CR10X, and CR23X dataloggers measures the frequency of the square wave with an analog channel.

Since fuel moisture doesn't change very rapidly, the sensor is typically measured only once an hour.

Instruction P27 measures the period of the output signal in microseconds. To prepare for the polynomial, the output is scaled by 0.001. A second-order polynomial is used to convert signal period to percent moisture content with the following constants:

C0 = -220.14
C1 = 365.89
C2 = -114.96

or, expressed as a second order polynomial
 $y = -220.14 + 365.89x - 114.96x^2$

CS505 FUEL MOISTURE SENSOR

5.1 CR10X EXAMPLE PROGRAM

A program to measure a CS505 fuel moisture sensor using the Period Averaging instruction P27 of a CR10(X), CR500, or CR23X datalogger. P27 is the preferred measurement technique with a Campbell Scientific, Inc. datalogger. P27 is not an option in the 21X datalogger.

:{CR10X}

<u>color</u>	<u>function</u>	<u>example CR10X Program wiring connections</u>
red	power	12V
black	ground	G
orange	control	C1
green	signal	1H (single-ended 1)
clear	shield	G

*Table 1 Program

01:	5	Execution Interval (seconds)	
1:	If time is (P92)		<i>Measure the CS505 once an hour.</i>
1:	0	Minutes (Seconds --) into a	
2:	60	Interval (same units as above)	
3:	30	Then Do	
2:	Do (P86)		<i>Turn on sensor by applying 5V to the enable lead.</i>
1:	41	Set Port 1 High	
3:	Period Average (SE) (P27)		<i>Measure the sensor's output period.</i>
1:	1	Reps	
2:	4	2 V Peak to Peak/200 kHz Max. Freq., Output Period	
3:	1	SE Channel	
4:	10	No. of Cycles	
5:	5	Timeout (units = 0.01 seconds)	
6:	1	Loc [FuelMoist]	
7:	0.001	Mult	<i>Prescaling for the polynomial.</i>
8:	0.0	Offset	
4:	Polynomial (P55)		<i>Convert sensor period to fuel moisture.</i>
1:	1	Reps	
2:	1	X Loc [FuelMoist]	
3:	1	F(X) Loc [FuelMoist]	
4:	-220.14	C0	
5:	365.89	C1	
6:	-114.96	C2	
7:	0.0	C3	
8:	0.0	C4	
9:	0.0	C5	
5:	Do (P86)		<i>Turn off the sensor.</i>
1:	51	Set Port 1 Low	
6:	End (P95)		

-Input Locations-

1 FuelMoist 5 1 2

5.2 21X EXAMPLE PROGRAM

A program to measure a CS505 fuel moisture sensor using the Pulse Count Instruction P3 of a 21X, CR10(X), CR500, or CR23X. The fuel moisture sensor is measured when flag 1 is set high. The measurement is made then flag 1 is set low.

;{21X}

<u>color</u>	<u>function</u>	<u>example 21X Program wiring connections</u>
red	power	12V
black	ground	⏏
orange	enable	control port 5
green	signal	pulse channel 1
clear	shield	⏏

*Table 1 Program

01:	1	Execution Interval (seconds)	
1:	If time is (P92)		<i>Set flag 1 high hourly, to measure CS505.</i>
1:	0	Minutes into a	
2:	60	Minute Interval	
3:	11	Set Flag 1 High	
2:	If Flag/Port (P91)		<i>If flag 1 is high, initiate the reading.</i>
1:	11	Do if Flag 1 is High	
2:	30	Then Do	
3:	Do (P86)		<i>Turn on the CS505 by applying 5 volts to the enable lead.</i>
1:	45	Set Port 5 High	
4:	Beginning of Loop (P87)		<i>Delay for complete count interval.</i>
1:	1	Delay	
2:	2	Loop Count	
5:	End (P95)		<i>End of loop to delay.</i>
6:	Pulse (P3)		<i>Determine the CS505 output frequency.</i>
1:	1	Reps	
2:	1	Pulse Input Channel	
3:	21	Low Level AC, Output Hz	
4:	1	Loc [CS505kHz]	
5:	0.001	Mult	<i>Convert to kHz</i>
6:	0.0	Offset	
7:	Do (P86)		<i>Turn off the CS505</i>
1:	55	Set Port 5 Low	
8:	Z=1/X (P42)		<i>Convert frequency in kHz to period in milliseconds.</i>
1:	1	X Loc [CS505kHz]	
2:	2	Z Loc [CS505mSec]	

CS505 FUEL MOISTURE SENSOR

9: Polynomial (P55)

Convert period to percent moisture content.

1:	1	Reps
2:	2	X Loc [CS505mSec]
3:	3	F(X) Loc [fuelmoist]
4:	-220.14	C0
5:	365.89	C1
6:	-114.96	C2
7:	0.0	C3
8:	0.0	C4
9:	0.0	C5

10: Do (P86)

Set flag 1 low

1:	21	Set Flag 1 Low
----	----	----------------

11: End (P95)

End

*Table 2 Program

02:	0.0000	Execution Interval (seconds)
-----	--------	------------------------------

*Table 3 Subroutines

End Program

-Input Locations-

1 CS505kHz 1 1 1

2 CS505mSec 1 1 1

3 fuelmoist 1 0 1

6. MAINTENANCE

The sensor element should be changed at least once a year with a new element in the spring. Since the characteristics of wood change so rapidly, more frequent replacements may be desirable.

To change the sensor element, loosen the Phillips head screws and replace with the new element. Tighten the screws after replacing the element.

APPENDIX A. EXPLANATION OF EXPERIMENTAL DATA

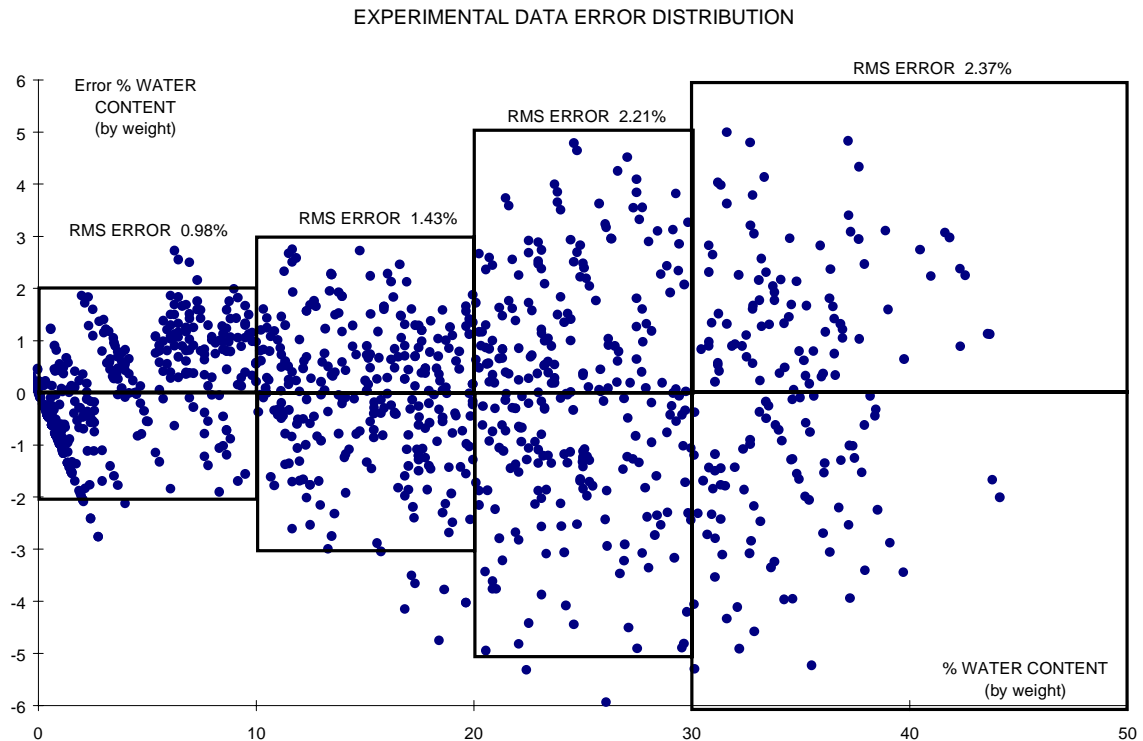


FIGURE A-1. Experimental Data Error-Distribution

Experiments were conducted to characterize measurement error and to determine the calibration polynomial coefficients used to convert the output signal to percent moisture content.

Populated circuit boards (before epoxy) oscillate with a period in the range of 0.6761 and 0.6780 milliseconds. In these experiments, three worst-case units were chosen. Only fuel moisture sticks that pass the standard rigorous selection criteria and then additional sorting for both oven-dry density and sorption qualities are chosen for production. For this experiment, 36 fuel moisture sticks were randomly selected from 300 production units. Electronic measurements were compared to actual stick weights. The sticks were soaked for 45 minutes, then after a five-minute dry, measured electrically and weighed every 10 to 60 minutes until they reached 15%. Then the sticks were placed in a 103°C oven for further drying; more measurements were taken. At each weigh

point the sticks were rotated and measured by each of the three electronic units. Over one thousand data points were measured for this calibration experiment.

The full scale range is broken into four sub ranges: 0-10, 10-20, 20-30, and 30-50 percent. The computed rms errors are shown in Table 1. For each range band an error band was determined in which more than 90 percent of all measurements fall (also shown in Table A-1 and Figure A-1).

APPENDIX A. EXPLANATION OF EXPERIMENTAL DATA

TABLE A-1. Accuracies at Measurement Ranges

<u>range</u>	<u>90% of all measurements</u>	<u>rms error</u>
0 to 10%	±2%	±1%
10 to 20%	±3%	±1.5%
20 to 30%	±5%	±2.2%
30 to 50%	±6%	±3%

*At least ninety percent of all experimental data fall within these error bands at the noted range divisions.

The above accuracy is a static accuracy derived at slow changing conditions with experimental data. In rapidly changing conditions (e.g., in the beginning of a rain event) the rate of response for each wood dowel differs. After sufficient time to equilibrate, the dowels will come to the same water content. This difference in rate of response is inherent in the traditional weighing fuel stick racks. The effects are lessened by the additional sorting of the dowels performed at the factory. Readings above 50% are caused by surface water on the probe or other external factors. Readings are mathematically limited to 70%.

The sensor error is the sum of three influences:

1. Error due to the variability and non-reproducibility of the response characteristics of the wood: density, sorption characteristics, resin content, etc.
2. Error due to the aging of the wood (cracking, discoloration, mass loss as resin evaporates). This effect is not a factor for new sticks.
3. Offset error due to the electronic circuitry interchangeability, this error is negligible over 10% fuel moisture.